

GTS-300 Operation Precautions

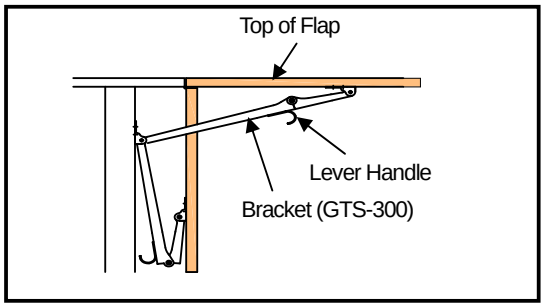

Opening the Flap

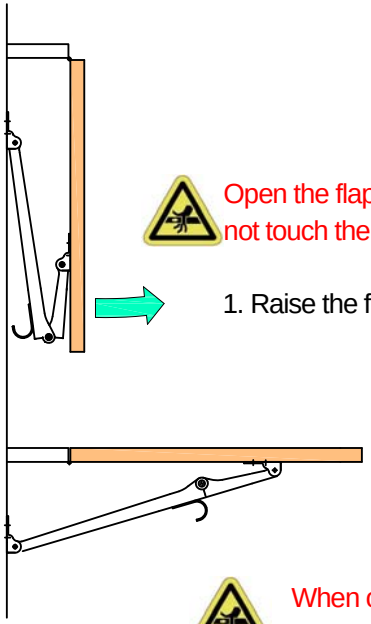


Open the flap by lifting on the flap itself. Please do not touch the bracket while opening.

1. Raise the flap by lifting upwards and outwards.

2. When the flap is horizontal and the bracket is fully extended, the bracket will automatically lock into place.

When open, do not lean or sit on flap.

Closing the Flap

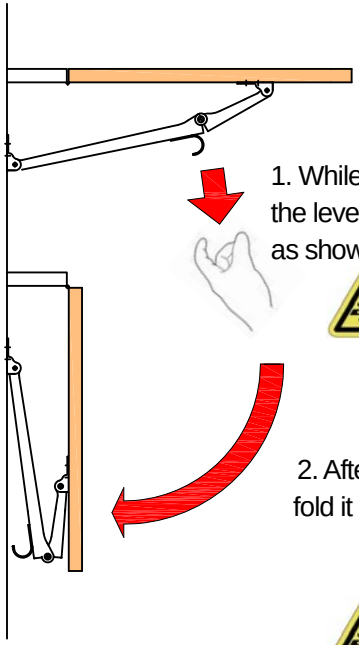

1. While supporting the flap with one hand, pull down and away on the lever handle to disengage the lock (in the direction of the arrow as shown).

Unlock the bracket by pulling on the lever handle only. Do not push/pull on the flap or any other part of the bracket when unlocking.

2. After unlocking the bracket, lower the flap gently and fold it into place.

Close by holding only the flap. Do not touch the bracket while closing.